



LAWRENCE
LIVERMORE
NATIONAL
LABORATORY

LLNL-TR-520312

Case for an Improved Effective-Atomic-Number for the Electronic Baggage Scanning Program

J. A. Smith, H. E. Martz, J. S. Kallman

December 14, 2011

Disclaimer

This document was prepared as an account of work sponsored by an agency of the United States government. Neither the United States government nor Lawrence Livermore National Security, LLC, nor any of their employees makes any warranty, expressed or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States government or Lawrence Livermore National Security, LLC. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States government or Lawrence Livermore National Security, LLC, and shall not be used for advertising or product endorsement purposes.

This work performed under the auspices of the U.S. Department of Energy by Lawrence Livermore National Laboratory under Contract DE-AC52-07NA27344.

Case for an Improved Effective-Atomic-Number for the Electronic Baggage Scanning Program

Jerel A. Smith
Jeffrey S. Kallman
Harry E. Martz Jr.

Lawrence Livermore National Laboratory
Livermore, CA 94551

Work performed on the
Science & Technology Directorate of the
Department of Homeland Security
Statement of Work
PR RSEN-08-00066

November 21, 2011

LLNL-TR-XXXXX-DRAFT



This document was prepared as an account of work sponsored by an agency of the United States government. Neither the United States government nor Lawrence Livermore National Security, LLC, nor any of their employees makes any warranty, expressed or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States government or Lawrence Livermore National Security, LLC. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States government or Lawrence Livermore National Security, LLC, and shall not be used for advertising or product endorsement purposes.

This work performed under the auspices of the U.S. Department of Energy by Lawrence Livermore National Laboratory under Contract DE-AC52-07NA27344.

Case for an Improved Effective-Atomic-Number for the Electronic Baggage Scanning Program

Jerel A. Smith
Jeffrey S. Kallman
Harry E. Martz Jr.

Lawrence Livermore National Laboratory
Livermore, CA 94551

1.0 Executive Summary

Z_{eff} , a parameter representing an “effective atomic number” for a material, plays an important role in the Electronic Baggage Scanning Program (EBSP) to detect threats in dual-energy computed tomography (CT) baggage-scanning systems. We believe that Z_{eff} , as defined and used on this program, does not provide the accurate representation of a material’s x-ray absorption properties that is needed by the EBSP.

We present the case for a new method that defines an effective atomic number for compounds and mixtures, which we refer to as Z_e . Unlike Z_{eff} , Z_e is tied by definition to the x-ray absorption properties of each specific material. Use of this alternative will provide a more accurate scale for calibrating Micro-CT and EDS systems against standard reference materials and will provide a more accurate physical characterization of the x-ray properties of materials evaluated on those systems.

This document,

- Describes the current usage of the Z_{eff} parameter
- Details problems entailed in the use of the Z_{eff} parameter
- Proposes a well-defined alternative— Z_e
- Proposes and demonstrates an algorithm for optimally associating Z_e with any specified compound or mixture
- Discusses issues that can impact the usefulness of an effective-Z model
- Recommends that, in order that the chosen effective-Z parameter not materially impact the accuracy of data produced by the EBSP program, the use of Z_{eff} be replaced by Z_e

2.0 Background

The key objective of this component of the EBS program is to provide information on materials, particularly HMEs, that EDS vendors can use to determine how each specific material would appear on their x-ray CT systems. X-ray CT systems measure an “apparent” linear-attenuation coefficient (LAC) for a material. In addition to the inherent x-ray properties of a sample (material density and atomic composition), the LAC depends on the thickness of the sample, the spectrum used to measure the sample absorption, and other physical characteristics of the measurement system.

The LAC, is defined by the classical Beer-Lambert law relating the attenuated intensity of a source, I , to the initial intensity, I_0 , a path-length, x , and the linear attenuation coefficient within that medium:

$$I = I_0 \text{Exp}[-\mu * x] \quad \text{Equation 1a}$$

where the LAC is represented by the symbol μ .

As we discuss the use of the LAC's in extracting information about HME specimens, it is helpful to keep in mind, that Equation 1a is really shorthand for a more complex expression. The hidden pieces are shown in Equation 1b.

$$I(Ex) = I_0(Ex) \text{Exp}\left[-\frac{\mu}{\rho}(Z, Ex) \int \rho(x) dx\right] \quad \text{Equation 1b}$$

We can see that the unattenuated spectrum, I_0 , and the attenuation coefficient are explicitly dependent on x-ray energy, Ex . The incoming spectrum, I_0 , is a continuum, not a single energy. The transmitted spectrum, $I(Ex)$ is not only reduced, but changed by the amount of material encountered as shown by the integral of the material density, ρ , along the path, x .

Note that the LAC, μ , can be equivalently expressed in terms of x-ray cross sections. This latter formulation is more appropriate to our approach, and will be used below to implement the proposed definition of the effective atomic number.

$$\frac{\mu}{\rho}(Z, Ex)\rho = \mu = \sigma_e(Z, Ex)\rho_e \quad \text{Equation 1c}$$

The mass-absorption coefficients, $\mu/\rho(Z, Ex)$, and the atomic cross sections, $\sigma_e(Z, Ex)$, have been systematically tabulated in x-ray absorption tables [1–3]. In this document, we are referring specifically to total or “narrow-angle” cross sections. This implies that x-ray measurements are made using well-collimated systems. For loosely collimated systems, the Beer's/Lambert law of Equation 1 begins to break down due to x-ray scatter in the radiographs.

A CT image is a spatial map of μ . Because the absorption of x rays is energy dependent, the spectrum evolves as the radiation penetrates a sample. Typically, the low-energy x-rays are preferentially absorbed, the average spectral energy increases, and thus μ decreases with depth, an effect referred to as "beam hardening."

The dependence of μ on spectrum means that it is also dependent on the system used to measure it. For an EDS to identify a material, its algorithms need to know what the LAC's of that material

will be on that specific system. It would be impractical to evaluate every HME of interest on every model of every EDS, so it is necessary to measure the x-ray properties of the sample on one “material-characterization” system, and to use that measurement to predict how that sample would appear on other “target” EDS systems. On the EBS program, the Micro-CT systems at TSL, TAFB and LLNL have been used as the material-characterization systems.

The Micro-CT systems are dual-energy systems. That is, each system measures LACs using two spectra: a high-energy spectrum and a low-energy spectrum. The LACs for both spectra are directly proportional to the electron-density of the sample and also depend in a complex way on the atomic-composition of the sample and on the shape of the spectrum used in the measurement (Equation 1b). The dependence on atomic composition of the LACs from the low-energy spectrum is much stronger than that of the high-energy spectrum, thus variations in the ratio of low-energy LACs to high-energy LACs (μ_{lo}/μ_{hi}) provide a measure of the atomic-composition of the specimen.

Some of the EDS are also dual-energy systems. However, while the low- and high-energy spectra for the Micro-CT systems are identical, or nearly so, the EDS spectra are neither the same as the Micro-CT spectra nor the same as those of other EDS systems. To use measurements taken on one characterization system to predict measurements on a second, non-identical, target system, it is necessary to develop a transfer function, or map, between measurements on the two systems.

An approach used on the EBS program for mapping the response of a dual-energy characterization system to a dual-energy EDS system has used the parameter, Z_{eff} (defined below) to characterize the atomic composition of materials. This report specifically discusses two different effective-atomic-number indices, Z_{eff} and Z_e , and uses a detailed notation to differentiate between the number as calculated from the composition of a material and a number that has been measured using a CT system. To limit confusion, we will begin by defining that notation along with a number of other symbols that are used throughout.

2.1 Definition of Symbols used in this Document

For a single element, its atomic number, Z , is unambiguous. For compounds and mixtures we can approximate the x-ray behavior of the material by an “effective atomic number.” Because we are discussing different measures of “effective Z ,” it is important to make the definition of the terms used in this document clear:

Effective Z: A number that uses a representative atomic number to approximate the energy-dependent absorption of a complex material. We use this term to refer generically to implementations of this concept. The EBS program has used Z_{eff} . In this document we propose an alternative, Z_e ; the various EDS vendors have their own methods.

Z_{eff} : is an effective Z that is currently used to describe known compounds using a traditional formula, Equation 2, where the a_i are the relative electron fractions contributed by the constituent atoms. That formula is somewhat arbitrary in that no such formula can be accurate over all materials and spectra. To date, on this program, we have used Z_{eff} to approximate the effective number of the reference materials used in the calibration assigning the value 3.8 to the parameter p . In this choice for p , we have not optimized the Equation 2 formula for either the spectra or materials of concern.

$$Z_{eff} = \sqrt[p]{\sum_i a_i Z_i^p}$$

Equation 2

- ^LZ_{eff}:** describes the atomic number of an unknown material as measured on the Micro-CT systems. ^LZ_{eff} is determined by comparing the spectral responses of the unknown material to those of the reference materials. ^LZ_{eff} is interpolated from the Z_{eff} numbers that have been assigned to the references. ^LZ_{eff} is a system-dependent parameter. Because the Micro-CT systems utilize nearly identical spectral responses, the ^LZ_{eff} from the Micro-CT systems are essentially the same. The response of a substantially different system can similarly be interpolated using LAC measurements from its reference standards. A system-specific mapping function then can be found to map values from the Micro-CT system to any other CT system so that sample measurements made on the Micro-CT system can predict measurements on that other system.
- Z_e:** is proposed as a more accurate parameter, and as a physically-defined x-ray model of known compounds (e.g. the reference materials), based on the calculated x-ray properties of those compounds. The Z_e model is designed to closely match the actual x-ray absorption of each material over the spectral region of interest. Per se, it removes the arbitrariness and lack of optimization entailed in using Z_{eff}.
- ^LZ_e:** If the recommended “Ze” method of characterizing the material were adopted, the Micro-CT determination of the x-ray properties of unknown materials, ^LZ_e could be calculated from the Z_e in exactly the same way ^LZ_{eff} has been interpolated from the Z_{eff}, except that the calibration scale of the reference materials will be based on Z_e rather than Z_{eff}. The notation would be changed from ^LZ_{eff} to ^LZ_e to mark the transition to the updated method.
- μ:** The linear attenuation coefficient in a material as defined in Equation 1. On the EBS program, the units of μ are mm⁻¹.
- μ_{lo}:** The linear attenuation coefficient in a material for the low-energy spectrum of a dual-energy system.
- μ_{hi}:** The linear attenuation coefficient in a material for the high-energy spectrum of a dual-energy system.
- Ex:** X-ray energy. In this document the x-ray energy is expressed in keV.
- {σ and ρ}:** In general, the linear x-ray absorption due to a thickness of any material is the product of a cross-sectional area σ (cm²/unit) and the density of the material ρ in the beam (units/cm²). “Units” can be electrons, atoms, or molecules, etc. In this paper we use moles of electrons as our “unit;” this allows us to work with “laboratory-sized” quantities of material. The cross-sections, σ, are strongly dependent on the atomic composition and on the x-ray energy. The densities, ρ, depend only on the material density.
- ρ_e:** Electron density per unit volume. In this document ρ_e is expressed in moles of electrons per cm³. ρ_e for an element can be simply calculated from the mass density ρ_m (g/cm³) by ρ_e = ρ_m * (Z/A), where Z and A are the atomic number and atomic weight. For a complex material the electron density is just the sum of contributions from the constituent elements:

$$\rho_e = \rho_m \sum_i w_i Z_i / A_i \quad \text{Equation 3}$$

where w_i is the numerical fraction of element i present in the compound, and Z_i and A_i are the atomic number and atomic weight of that atom.

σ_e : the x-ray cross-section for a specified atomic number, Z , and a given number of electrons. In this document σ_e is expressed in cm^2 per mole of electrons. σ_e depends strongly on the atomic number of a material, Z , and on the x-ray energy, E_x . For clarity, this may be shown expressly as $\sigma_e(Z, E_x)$. In this document σ_e is interpolated from the Livermore Evaluated Photon Data Library [1] with the conversion of the unit of charge from a single electron, to a mole of electrons. For a complex material:

$$\sigma_e = \sum_i b_i \sigma(Z_i) \quad \text{Equation 4}$$

where $\sigma(Z_i)$ is the published cross section of the element, Z_i , and b_i is the fraction of electrons contributed by the element Z_i .

σ_{Ze} : The x-ray cross-section (cm^2 per mole of electrons) for a compound or mixture with an effective atomic number Z_e . For clarity, this may be shown expressly as $\sigma_{Ze}(Z_e, E_x)$.

2.1 How Z_{eff} has been used on this program to characterize HMEs

The current program strategy to predict the EDS measurements on an HME based on Micro-CT measurements can be summarized as follows (the details of steps 4–6 are elaborated in Section 2.2):

Calibrate the characterization and target systems:

1. Establish a set of reference materials whose effective Z and densities span the compositional range of materials of interest.
2. Assign each reference material an “effective atomic number” parameter, Z_{eff} , to represent its material composition.
3. Measure the dual-energy LACs. μ_{lo} and μ_{hi} , for each reference material on the characterization system and on each target system.
4. For each system, approximate the relationship between the Z_{eff} of the references and the measured LAC ratio ($\mu_{\text{lo}}/\mu_{\text{hi}}$) by an interpolating polynomial.

Measure the μ_{hi} and $^L Z_{\text{eff}}$ of the HME:

5. Measure the LACs of the HME on the characterization system.
6. Use the Micro-CT polynomial function from step 4 to interpolate $^L Z_{\text{eff}}$ of the HME from the $\mu_{\text{lo}}/\mu_{\text{hi}}$ ratio.

Calculate the EDS μ_{lo} and μ_{hi} of the HME from the $^L Z_{\text{eff}}$ and μ_{hi} of the Micro-CT:

7. Use the EDS polynomial function from step 4 to interpolate the EDS $\mu_{\text{lo}}/\mu_{\text{hi}}$ ratio from the measured Z_{eff} .
8. Obtain the μ_{hi} of the EDS from that of the Micro-CT (for improved accuracy, this relationship can be calibrated).
9. Calculate the μ_{lo} of the EDS from its μ_{hi} and the ratio from step 7.

In this paper, we are specifically concerned with the techniques used to implement Step 2. As we will show, Z_{eff} is defined in a way that makes it an incomplete, ambiguous, and imprecise representation of the x-ray properties of complex materials. By “complex materials,” we refer to any combination of molecular compounds or mixtures that consists of more than one element. Because Z_{eff} lies at the core of the response-mapping strategy, these deficiencies affect the accuracy with which measurements on the Micro-CT system can predict measurements on the EDS.

2.2 Measurement of $^LZ_{\text{eff}}$ based on the LACs and Z_{eff} 's of the reference samples

The experimental configuration of the Micro-CT systems provides two physically separate layers for the measurements[4]. The HME specimen is contained in a bottle on the top layer of a rotating sample holder (the “carousel”). The (nominally) ½-inch diameter reference samples are on the lower layer. A number of reference samples were chosen for use on this program [5]. For the measurements described here, each layer is imaged using an x-ray fan collimated through a narrow slit. The selected materials, and their assigned Z_{eff} 's are shown in Table 1.

Table 1. *A list of the reference materials used on the Micro-CT and their assigned Z_{eff} parameters. The ethanol and water are in polypropylene bottles.*

Material	Z_{eff}	Nominal Formulation
Graphite	6.00	C
Ethanol	6.53	95% Denatured Ethanol
Delrin	7.07	H ₂ CO
Water	7.54	H ₂ O
Teflon	8.50	CF ₂
Aluminum	13.00	6061 aluminum alloy

The interpolation of the measured $^LZ_{\text{eff}}$ number for a hypothetical HME is illustrated in Figure 1. The measurements from the reference samples are shown as blue and red data points. Their measured LAC ratios ($\mu_{\text{lo}}/\mu_{\text{hi}}$) and assigned Z_{eff} 's are given on the horizontal and vertical axes respectively. The interpolation function is implemented as two separate polynomials (one each for the low- and high- Z_{eff} ends of the data); the Delrin measurement is common to both fits[6].

For this graph, actual Micro-CT data have been used for the reference measurements. However, the HME measurement is hypothetical. We have assumed that the measured $\mu_{\text{lo}}/\mu_{\text{hi}}$ ratio for the hypothetical sample is 1.8. The $^LZ_{\text{eff}}$ for this specimen is then interpolated from the upper (red) curve as 9.74. The notation $^LZ_{\text{eff}}$ indicates that this is an empirically measured number that has been interpolated from a measurement scale based on the calculated parameter Z_{eff} .

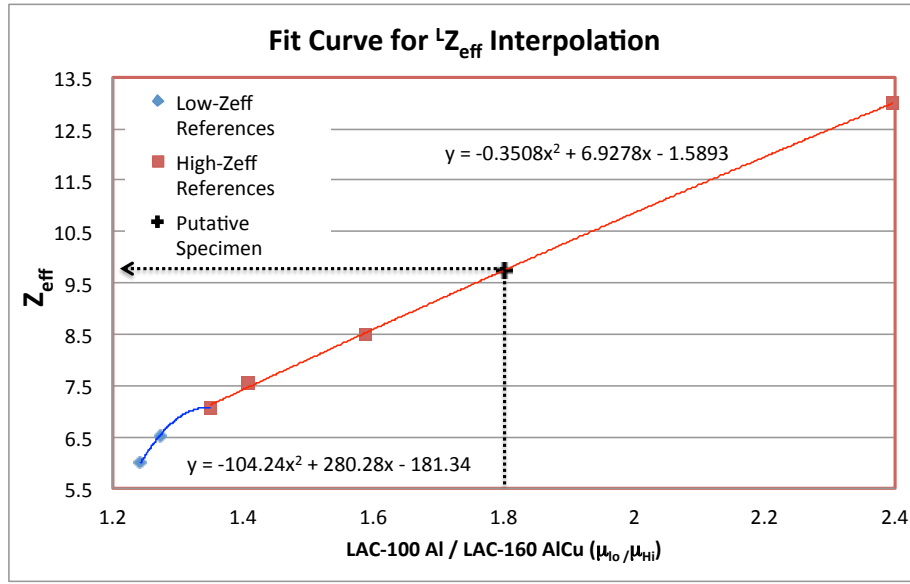


Figure 1. The method for measuring the LZ_{eff} of an HME (steps 4–6 in the text) is illustrated in this graph. The interpolation formulas for the low- and high- ends of the data are shown explicitly. The reference measurements are taken from LLNL Micro-CT data. The measurements on the “HME sample” are hypothetical.

3.0 Discussion of the Z_{eff} Parameter

One of the key requirements for x-ray detection of HME is to provide a representation of the chemical composition of the material as it appears in x-ray measurements. Every element (referred to by its atomic number, Z) has a unique signature in the way it absorbs x-ray radiation. For example, high- Z elements have greater absorption, particularly at the lower x-ray energies. A compound or mixture of materials exhibits absorption that is a blend of the absorption from its constituent elements and will, in its energy dependence, resemble elements somewhere between the highest and lowest Z 's present in the mixture. Because of the complexity of components involved in x-ray absorption, it is not possible to exactly represent any compound material as a single element, or using any single parameter. However, it can be possible, and useful, to approximate the absorption by a single parameter *provided that parameter is associated with a model that specifies the energy-dependent absorption of that material, and that provides a means to optimize and evaluate the accuracy of the model.*

The technique that has been used to date on this program has its historical roots in medical x-ray technology. In 1946, to estimate (without doing detailed and computationally-intensive, calculations) where a particular material's absorption properties would fall on an “effective- Z ” scale, F. W. Spiers [7] proposed the Equation 2 expression with the power parameter, $p=2.94$.

$$Z_{eff} = \sqrt[p]{\sum_i a_i Z_i^p} \quad \text{Equation 2}$$

The a_i are the relative electron fractions contributed by the constituent atoms. Since that time, this formula has been used as a convenient “rule-of-thumb,” though the exact choice of the exponent, p , has varied from observer to observer. Indeed, for best results, p should be chosen to

fit the desired range of materials and spectra [8–12]. Given an optimal selection of p , this method has proven useful in the medical field for interpolating properties on specific systems and within the relatively narrow, and low- Z , range of materials of biological interest. If higher- Z components are present in the materials, it becomes very difficult to fit Equation 2 to materials of interest. For example, McCullough [9] warns that:

*... even for the specific sub-components of the cross-sections, no single formula of the...
<< Equation-2 >> ... form can describe the variations of those sub-components ...to the
accuracy desired by any analysis relevant to CT scanning.*

As discussed above, the strategy for the EBS has been to analytically interpolate an effective $^LZ_{\text{eff}}$ for an HME based on LAC ratios measured on reference materials, notably graphite, ethanol, Delrin, water, Teflon, and aluminum. The independent variable (Z_{eff}) for the references was assigned using the Z_{eff} formula (Equation 2) with the power $p = 3.8$, as suggested by TSL. The interpolated effective- Z for the HME is called $^LZ_{\text{eff}}$. Unless otherwise specified, all Z_{eff} values in this document are calculated using $p = 3.8$.

The use of the Z_{eff} equation to provide a characterization of the x-ray properties for complex materials raises several issues.

The use of the Z_{eff} equation is inherently problematic

The Z_{eff} equation was introduced as a computational tool to estimate the x-ray absorption properties of complex materials at a time when detailed computation of the energy-dependent coefficients would have been difficult and expensive. It has likely not evolved, because its primary constituency, medical physics, has not needed to provide an accurate scale for as broad a range of materials as addressed by this program. Issues with the use of this formula include:

1. **Any selection of the exponent “ p ” in Equation 2 will not fit all compounds equally well.** The selection of “ p ” is a compromise. If the spectral and compositional range is limited, a “best value” can be chosen. Evaluating the accuracy of that choice is problematic because there is no specified relationship between Z_{eff} and the x-ray properties (see point 4 below). As new HME’s become of interest, and particularly if more high- Z components are used in the HME samples, the choice of “ p ” may need to be revisited. That would be disruptive to the continuity of the measurement strategy.
2. **The currently selected exponent, $p=3.80$, is not appropriate for representing HME.** As shown in McCullough [9] an exponent of 3.8 is only representative of the Z -dependence of the photoelectric absorption, and will consistently over-estimate the Z_{eff} for other materials with high- Z constituents. Typical HME are dominated more by Compton than photoelectric absorption and an optimal compromise would use a smaller exponent.
3. **The calculated Z_{eff} is an inherently ambiguous indicator of the x-ray absorption properties of materials.** The simple way to see this is to look at Equation 2. An almost unlimited number of constituents could be compositionally adjusted to fit a specific Z_{eff} number as long as that number is somewhere between the lowest and highest Z of the constituents selected. These varied compounds will, however, each have different x-ray absorption properties.
4. **There is no defined way to get from the calculated “ Z_{eff} ” to the x-ray absorption properties of the material.** We need the “effective- Z ” to describe physical properties—

the energy-dependent x-ray absorption—of an HME. Without a definition of the x-ray absorption that is specified by the Z_{eff} we can say neither what those properties are, nor whether the selected number accurately describes those properties. Put simply, we do not have a physical model for Z_{eff} .

There is a considerable overlap between points 3 and 4, and it is worth illustrating the issue. For example, few would dispute that a material with an effective Z of 10 ought to appear the same as a compact sample of the element neon ($Z=10$). For example, if a small amount of iron is added to a carbon substrate, to raise the Z_{eff} of that sample to 10.0, the absorption cross sections of that material ought to closely track the cross sections of neon.

If iron is added to a carbon base, with a weight fraction of 2.44%, the Z_{eff} calculated by Equation 2 (using $p=3.8$) is 10. In Figure 2, the total x-ray cross sections of neon (red line) and the putative $Z_{\text{eff}}=10$ compound (blue line) are compared; clearly, the low-energy absorption is much lower in the putative composite than in the neon (the black dotted line will be discussed later).

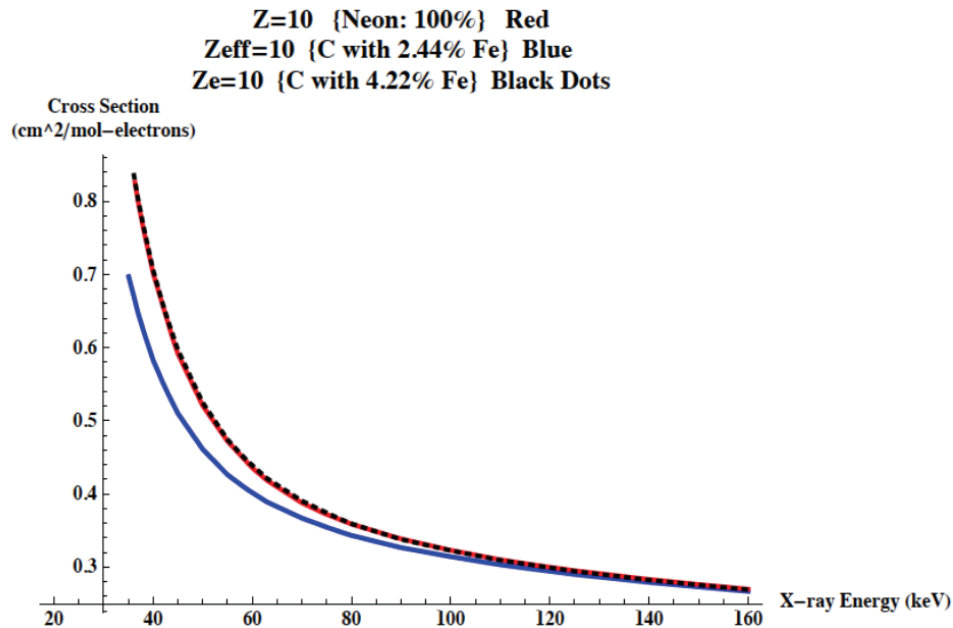


Figure 2. The x-ray cross-sections are compared for Neon ($Z=10$) and for a carbon composite having 2.44% iron by weight ($Z_{\text{eff}} = 10$). At the low-energy end of the graph, the cross section for the composite is about 30% lower than that of the Neon. Clearly these material responses are significantly different. The cross section for $Z_e = 10$, calculated using the proposed alternative technique (black dots), closely follows that of neon.

The contrast between the elements used in the mix ($Z = 6$ and 26) is large, but it illustrates the point: Z_{eff} is ambiguous. Any given Z_{eff} number can represent a range of materials and a range of x-ray properties. This means that Z_{eff} cannot precisely specify the x-ray properties of the references, therefore, $^LZ_{\text{eff}}$, the measurement of an HME that is interpolated from the Z_{eff} , cannot accurately convey the properties of that material to an EDS vendor.

An exponent “ p ” in Equation 2 could be found to make this particular choice of ingredients match, however another selection of materials would then present a poor match. The fundamental point is that Equation 2 is not a physical model for a material’s response— it

provides no formula for calculating a unique x-ray response for a specified Z_{eff} , and no means to verify that response.

In the next section, we present an alternative method for associating an effective atomic number, Z_e , with a specific material. Using that approach, which is based on a physical model, we find that a Z_e of 10.0 corresponds to the addition of 4.20% iron by weight to the carbon. In Figure 2, it is clear that the cross-section for a C/Fe material with $Z_e = 10$ (black dots) is almost indistinguishable from that of neon.

4.0 An Alternative Approach to Selecting the “Effective Z”

There is a simple alternative, Z_e , that eliminates the problems in the previous section resulting from the Z_{eff} formulation. There are two steps:

- Provide a physically meaningful definition for the effective Z , Z_e , and for the corresponding x-ray cross-section: $\sigma_{Ze}(Z_e, Ex)$.
- Provide an algorithm for determining Z_e for an arbitrary known compound or mixture of elements.

4.1 Define Z_e and $\sigma_{Ze}(Z_e, Ex)$

In x-ray physics, a material is described by its energy-dependent cross-section and electron density. Therefore, to have any physical meaning, Z_e must be defined by specifying $\sigma_{Ze}(Z_e, Ex)$.

Our definition of $\sigma_{Ze}(Z_e, Ex)$ is extremely simple, it is a linear interpolation between $\sigma_e(Z, Ex)$ and $\sigma_e(Z+1, Ex)$ where $\sigma_e(Z, Ex)$ is interpolated directly from any standard set of x-ray absorption tables [e.g. 1–3]. To be specific:

- For integer Z_e , the energy dependent x-ray cross-section of a material is exactly that of the corresponding element with atomic number Z , i.e.:

$$\text{Integer } Z_e: \quad \sigma_{Ze}(Z_e, Ex) = \sigma_e(Z_e, Ex) \quad \text{Equation 5a}$$

- For non-integer Z_e , the cross-section, σ_{Ze} is obtained from a proportionate mixture of the cross-sections from the immediately adjacent elements. For example, a Z of 8.3 would be a 70/30 blend of Oxygen ($Z=8$) and Fluorine ($Z=9$). The x-ray cross-sections for this material can then be calculated:

$$\sigma_{Ze}(8.3, Ex) = 0.7\sigma_e(O, Ex) + 0.3\sigma_e(F, Ex)$$

This definition can be written more formally. If we express the Z_e as a real number with an integer part (Z) and a fractional part (frac), then,

$$\text{Non-integer } Z_e: \quad \text{Equation 5b}$$

$$\sigma_{Ze}(Z.\text{frac}, Ex) = (1 - \text{frac}) * \sigma_e(Z, Ex) + \text{frac} * \sigma_e(Z + 1, Ex)$$

In practice, only Equation 5b is required, because, if Z_e is an integer, Equation 5b reduces to Equation 5a. Note that “frac” refers to the fraction of electrons, rather than the fraction of atoms, contributed to the material from the $Z+1$ element.

Equation 5b defines Z_e : *A material with an effective atomic number, Z_e , has the energy-dependent cross-section of Equation 5b.*

Note that this definition of Z_e is not an approximation. It is a specific definition in terms of physical parameters. It is valid over the same range of parameters as the x-ray absorption tables from which it is interpolated. Our knowledge of the x-ray cross-section of Z_e , is neither more nor less accurate than those tables, which express the current knowledge of x-ray interaction probabilities.

Combining Equations 1, 4, and 5 for compounds, the familiar exponential attenuation of x-ray intensity with thickness, x , can be written:

$$I(Ex) = I_0(Ex) \exp[-\sigma_{Ze}(Z_e, Ex) \int \rho_e(x) dx] \quad \text{Equation 6}$$

Two obvious questions arise:

1. How do you find an optimal Z_e for a specified compound or mixture?
2. When can the x-ray properties of any specific material be accurately approximated by Z_e (or any other effective- Z)?

4.2 Calculating Z_e for an Arbitrary Compound or Mixture

For compounds and mixtures of elements, $\sigma(Ex)$ is just the proportionate sum of the cross sections of the constituent atoms. Elaborating on Equation 4, for a material with N types of atoms, with atom Z_i present in the proportion n_i :

$$\begin{aligned} \sigma(\text{material}, Ex) &= \sum_i^N b_i \sigma(Z_i, Ex) \\ b_i &= n_i Z_i / \sum_{i=1}^N n_i Z_i \end{aligned} \quad \text{Equation 7}$$

As an example, for water, H_2O , $N = 2$, $Z_1 = 1$, $Z_2 = 8$, $n_1 = 2$, $n_2 = 1$.

and
$$\sigma(\text{water}, Ex) = \frac{2}{10} \sigma(H, Ex) + \frac{8}{10} \sigma(O, Ex)$$

The procedure for finding Z_e is then conceptually simple, the best Z_e provides the best agreement between $\sigma_{Ze}(Z_e, Ex)$ and $\sigma(\text{material}, Ex)$. Another way to state the principle is “use the Z_e that will provide the best match for the (Equation 7) calculated cross-section of the known material.”

A straightforward approach would be to use a Z_e that has the best least-squares-fit to the cross-section over the x-ray range of interest. However, we suggest using a finesse here that provides a more robust result.

Recall that any effective- Z , including Z_e , can only provide an approximation to the energy-dependent cross-section of a compound. For any compound, that approximation will eventually fall apart at the lowest energies largely because the ratio of the coherent and photoelectric cross-sections differs between the actual compound, and that calculated via the Z_e definition. That discrepancy will occur at higher energies if the material is a mixture of very-high and very-low- Z elements. The combination of the high- Z (iron) with the low- Z (carbon) in Figure 2 was deliberately chosen to emphasize that effect.

However, we are using Z_e to describe the *transmission* of materials over a broad, but finite, spectral region. However, the transmission of an object rapidly decreases at the lowest energies. If there is significant x-ray transmission at the lowest energies, we would like to find the best compromise that includes those low energies. But, where there is very little transmission at low energies, we want to decrease the weight given to the lowest energies.

The way we have handled this is to select Z_e to obtain the best least-squares-fit for the *transmission* of x rays through a material of moderate thickness. For the EBS program 2.5 g/cm² of material (essentially 1-inch of water) seems appropriate, and has been used for the calculations in this paper. Note that the choice of thickness is not at all critical, however allowing the material absorption to weight the least-squares fit provides a self-adjusting cutoff for the lowest energies used in the calculation whenever higher-Z constituents are present. This is illustrated in section 4.3. Use of transmission weighting also de-emphasizes the highest energies where there is less absorption and little Z-dependence in the absorption.

It is also important to apply the optimization over an appropriate spectral region. For EBS applications, the combination of source filtering and object attenuation transmits little radiation below 30 keV, and typical peak source energies are 160 keV, so we have done our optimization over a range of 30–160 keV.

The results of applying this algorithm to Teflon are illustrated in Figure 3, where a Z_e of 8.41 is shown to closely fit the transmission of Teflon across the selected range. As shown earlier in Figure 2, the energy-dependent cross section for an Fe/C mixture, calculated using this algorithm, also fits the Z_e description very closely.

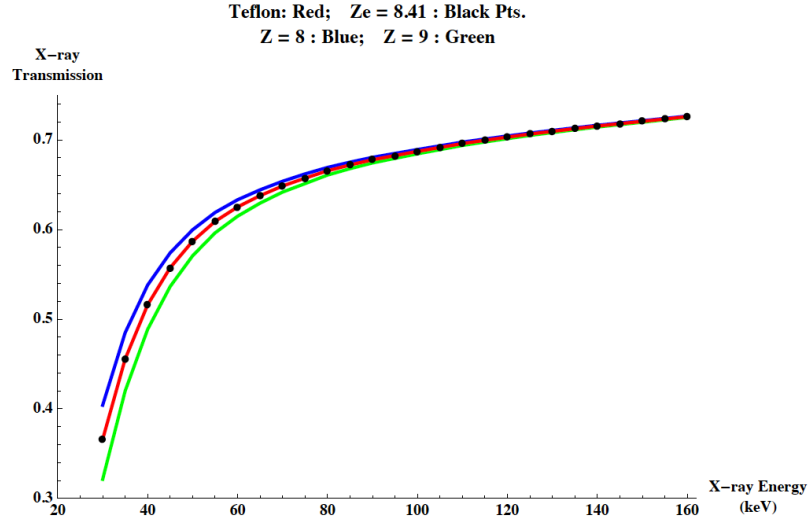


Figure 3. The x-ray transmission through a (2.5 g/cm²) sheet of Teflon (red) is closely matched by the transmission calculated for Z_e of 8.41 (black points). For comparison, transmissions through the same areal mass of Oxygen ($z=8$) and Fluorine ($z=9$) are shown.

4.3 Range of Applicability of Effective-Z Models

Z_e , or any effective-Z, is an approximate description of a material. For many materials, and spectral regions—and for most materials of interest to the EBS Program—it can be an excellent approximation of the energy-dependent x-ray absorption. Two situations may present problems.

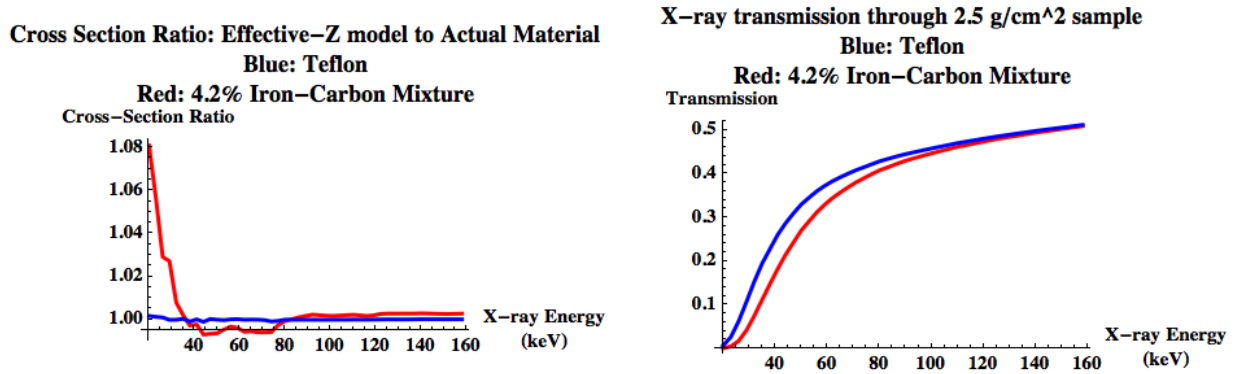


Figure 4. For Teflon, the effective-Z provides an excellent approximation to the cross-section over a broad range of energies. However, for the fictional Fe/C mixture analyzed in the text, $Z = 10$ is accurate down to about 35 keV. Below 30 keV, the cross-section ratio quickly diverges. Optimizing Z_e according to the transmission through a material sample, effectively eliminates sensitivity below 30 keV.

First, for any complex material, the effective-Z model will have a low-energy limit, below which the actual cross section and effective-Z cross section diverge. Figure 4 illustrates this issue for Teflon and for the iron/carbon mixture that was discussed above. The left panel of this figure plots the ratio of the effective-Z models, $\sigma_e(Z_e, E_x)$ to the calculated cross-section, $\sigma(\text{material}, E_x)$, for the actual materials. For Teflon, which is composed of the relatively low-Z materials carbon and fluorine, the cross sections match very closely down to 20 keV. For the posited iron/carbon mixture, the ratio diverges below 35 keV.

However, the algorithm used to optimize Z_e , calculates transmission differences through a 2.5 g/cm² sample. As shown in the right panel of Figure 4, the transmission through the iron/carbon mixture cuts off at about 30 keV, so the ratio divergence would have little effect on the calculated value of Z_e . In the field, EBS systems would only see a difference between the effective-Z model and the material for thin sheets, unshielded by other material, and viewed perpendicular to the surface of the sheet. Thus, even for a fairly radical high-Z/low-Z mixture, the Z_e model remains robust. At some point, as the contrast between the constituent materials increases, the model will break and an effective-Z model will not be useful.

The hypothetical iron/carbon sample, is just at the threshold where an effective-Z model becomes inappropriate, and serves as an illustration that, if we use an effective-Z model for the materials being characterized, we need to be vigilant as small amounts of high-Z elements are added to the compound.

The second problem that may arise is the inclusion of elements with absorption edges in the middle of the observing spectrum. The k-absorption edge of tin ($Z=50$) is just below 30 keV and should not present a problem. However elements significantly above that, such as lead or tungsten, could present a “jagged” transmission characteristic that would be very sensitive to the low-energy cutoff of the probing spectrum. Again, in that situation, an effective-Z model would not be useful. Like any tool, effective-Z models need to be used thoughtfully.

5.0 Are the proposed changes Better and are they “Significant?”

Z_e is *qualitatively* “better” than Z_{eff} in that the Z_e calculation provides a model to define the x-ray transmission properties of the material having that effective atomic number. Z_{eff} is, in fact, mathematically ambiguous. Z_e provides a valid single-valued physical model for every material.

Z_e is *quantitatively* better because it provides an accurate approximation to the x-ray transmission for *any* specified material. Its accuracy is built in by using the best-fit algorithm in its implementation.

Table 2. Comparisons of the Z_{eff} that are used on the current program and the improved Z_e values using the approach outlined above.

Material	Z_{eff}	Z_e	Difference	Formulation
Ethanol	6.53	6.35	- 0.18	100% Ethanol
Delrin	7.07	6.99	- 0.12	H ₂ CO
Water	7.54	7.40	- 0.14	H ₂ O
Teflon	8.50	8.41	- 0.09	CF ₂

Evaluation of Micro-CT system performance has shown measurement consistency for the μ_{lo} and μ_{hi} on the order of 0.6% and 0.1% respectively [13]. Additionally, evaluation of HME on this program has indicated the need to achieve measurement precision for μ_{hi} on the order of ½% [14]. From the slope of the upper segment of the Figure-1 graph, we can see that 0.6% variation in the measurement of the LAC ratio, corresponds to a variation in the Z_{eff} of about 0.04.

Table 2 provides a perspective on the magnitude of the adjustments resulting from using the Z_e process for calculating the “effective-Z”. The table assumes that the nominal molecular compositions are correct. If the program objective is to measure material properties, the differences exceed the figure-of-merit ($\Delta Z \sim 0.04$). This suggests that, at present, the accuracy and consistency of our “Zeff ruler” is not as precise as our LAC measurements and that a more accurate calibration would be appropriate.

If the number $^LZ_{eff}$ is intended to convey information about a specific sample, its ambiguity and lack of precision does not seem appropriate for its role. Note that the ambiguity becomes greater when higher-Z elements are present in the sample.

Advantages to the Proposed Definition of Z_e

- Accuracy: The definition of Z_e optimizes the effective-Z for each material.
- Flexibility: If, and when, new HME are encountered, the selected algorithm does not need to be adjusted. The technique, by its definition, provides an optimized description for each material.
- Specificity: The effective atomic number, Z_e , along with the areal density of a particular sample, ρ_e , uniquely specifies the x-ray absorption for each material.

6.0 Summary and Recommendations

- The Z_{eff} parameter does not accurately describe the x-ray properties of materials. An alternative, Z_e , provides a more accurate material description.
- To assure that the choice of an effective-atomic number parameter does not significantly impact the accuracy of data produced on this program, we recommend that the use of Z_{eff} be replaced, and that the more accurate Z_e be used instead.
- At some point, the EBS program will need to move to a more precisely defined set of reference materials to serve as the measurement standards for characterization of HME. That would provide an opportunity to move the program to the use of the more accurate Z_e parameter (See Appendix).

7.0 References and End Notes

- 1) D.E. Cullen, S.T. Perkins, and J. A. Rathkopf, *The 1989 Livermore Evaluated Photon Data Library (EPDL)*, UCRL-ID- 103424, Lawrence Livermore National Laboratory (1990).
- 2) D.E. Cullen, J. H. Hubbell, and L. Kissel, *EPDL97: The Evaluated Photon Data Library '97 Version*, UCRL—50400, Vol. 6, Rev. 5, Lawrence Livermore National Laboratory (1997).
- 3) J. H. Hubbell, and S. M. Seltzer, *Tables of X-Ray Mass Attenuation Coefficients and Mass Energy-Absorption Coefficients from 1 keV to 20 MeV for Elements Z = 1 to 92 and 48 Additional Substances of Dosimetric Interest*, **NISTIR 5632**, 1996:
<http://www.nist.gov/pml/data/xraycoef/index.cfm>
- 4) J. A. Smith, D. J. Schneberk, J. S. Kallman, H. E. Martz, Jr, d. Hoey, r. Krauss, r. Klueg, *Documentation of the LLNL and Tyndall Micro-Computed-Tomography Systems Micro CT* , LLNL-TR-421377, 2011.
- 5) R. Krauss, R. Klueg, *Standard Operating Procedure: Industrial Computed Tomography System Data Collection of Home-Made Explosives*, DHS/STD/TSL-XX-XX, 2009.
- 6) J. S. Kallman, D. J. Schneberk, H. e. Martz, Jr., *Ratio of Two Energy Spectra Method and Reference Materials to determine Effective Z*, LLNL-TR-XXXX (Draft), 2009.
- 7) F. W. Spiers, *Effective Atomic Number and Energy Absorption in Tissues*, Br. J. radiol.,19, 52, 1946.
- 8) J Weber, and K. J. van den Berge, *The effective atomic number and the calculation of the composition of phantom materials*, Br. J. Radiol., 42, 378-383, 1969.
- 9) E. C. McCullough, *Photon attenuation in computed tomography*, Medical Physics, Vol. 2. 6, Nov/Dec, 1975
- 10) D. R. White, *An Analysis of the Z-dependence of Photon and Electron Interactions*, Phys. Med Biol., 1977, Vol. 22, 219-228, 1977.
- 11) N. C. Yang, P.K. Lechner, and W. G. Hawkins, *Effective atomic numbers for low-energy total photon interactions in human tissues*, Medical Physics, Vol. 14, No. 5, Sep/Oct 1987.
- 12) B. J. Heismann, J. Leppert, and K. Stierstorfer, *Density and atomic number measurements with spectral x-ray attenuation method*, Journal of Applied Physics, Vol. 94, No. 3, 2073–79, 2003.
- 13) J. S. Kallman, H.E.Martz and W.D. Brown, *MicroCT Reference Materials QA Windows*, LLNL-PRES-489954-DRAFT slide 7, July 2011.
- 14) H. E. Martz, Jr. C. R. Crawford, J. S. Kallman, *Set 1b Group 1 Information*, LLNL-MI 465052, 2011.

8.0 Appendix: How the Proposed Definition of Z_e Impacts the Current HME Program

- In conjunction with obtaining chemical assays of the “as deployed” reference materials, the effective-Z would be recalculated using the Z_e definition. The magnitude of the impact on previous data should be assessed in view of those results.
- To bring previous work in line with the improved calibrations, the work based on the Z_{eff} calibrations could be updated, however, it may be adequate to simply provide a “correction function” to adjust previous Z_{eff} results to the more accurate Z_e .
- For the immediate future, the effective-Z of the HME would be interpolated using the current interpolation technique, but with the assigned effective atomic number of the references based on the more accurate Z_e scale calculated using accurately assayed reference materials. These would be referred to as LZ_e , where LZ_e is Z_e measured using the IDD interpolation technique. For materials with known composition, Z_e can be calculated directly. That is, the x-ray cross section can be calculated based on published data [1–3].

Effect of Changing the Effective-Z on Data Acquisition

Micro-CT data acquisition is unchanged when we recalibrate the effective atomic number of our references.

Effect of Changing Effective-Z on Image Reconstruction and Object Segmentation

CT reconstruction and segmentation remain unchanged.

To effect the change in computing LZ_e will require replacing the current Z_{eff} values for the references in the characterization template spreadsheet with the Z_e values determined by the technique described above and based on the chemical assays of the as-deployed reference materials.